

The role of a novel oral appliance therapy device on pharyngeal pressure swings and CPAP requirements during sleep in obstructive sleep apnea: **A pilot study**

Jason Amatoury^{1,2}, Benjamin Tong¹, Chinh Nguyen¹, Irene Szollosi³, Danny J. Eckert^{1,2}

¹ Neuroscience Research Australia (NeuRA), Sydney, Australia.

² School of Medical Sciences, University of New South Wales, Sydney, Australia.

³ Oventus Medical Ltd, Brisbane, Australia.

INTRODUCTION:

Oral appliance (OA) therapy is often an effective alternative to continuous positive airway pressure (CPAP) for the treatment of obstructive sleep apnea (OSA). However, OA treatment efficacy varies and is often poorly tolerated in people with high nasal resistance. A new OA therapy device that incorporates an opening to the oral cavity (Oventus, O₂Vent T) allows breathing through the device airway, which may reduce the high inspiratory pressures required to drive air through the pharynx in people with nasal obstruction. The goals of the current study were to: 1) assess pharyngeal pressure swings during sleep with and without the OA therapy device and 2) determine the effect of the device on the CPAP requirements to minimize pharyngeal pressure swings and abolish residual events.

METHODS:

Four individuals were studied overnight in the sleep physiology laboratory (3 male; age: 43-62 yrs, BMI: 28-33 kg/m²). In addition to standard polysomnography, subjects were fitted with a nasal CPAP mask and pneumotachograph to quantify airflow. Choanal pressure (Pcho) and epiglottic pressure (Pepi) were measured using pressure transducer-tipped catheters. Nasal resistance was quantified during quiet nasal breathing awake $[(P_{\text{mask}} - P_{\text{cho}}) / \text{flow} @ 200 \text{ml/s}]$. Nasal CPAP was carefully titrated during NREM sleep to determine "therapeutic CPAP" level. Participants were studied under the following conditions during supine NREM sleep: 1) no OA and no CPAP (baseline), 2) OA only, 3) CPAP only, and 4) OA and CPAP combination therapy. The degree of mandibular advancement with the OA therapy device was sub-optimal to allow expression of residual events that required

combination OA and CPAP therapy. The apnea/hypopnea index (AHI) and nadir Pepi swings were determined during each condition. CPAP levels with OA therapy to achieve nadir Pepi values equivalent with therapeutic CPAP without the OA was also determined.

RESULTS:

Awake nasal resistance ranged between 2.8 and 20.6 cmH₂O/ml/s (12.3±8.2 cmH₂O/ml/s, mean±SD). 3/4 participants had high nasal resistance (>3 cmH₂O/ml/s). Baseline AHI was 37±35 events/hr, which decreased with OA therapy to 8±10 events/hr. Average nadir Pepi swings during baseline NREM sleep were -8.5±2.5 cmH₂O, falling to -4.1±1.6 cmH₂O with OA therapy. The therapeutic CPAP level required to abolish respiratory events during NREM sleep without OA therapy was 6.8±2.4 cmH₂O with corresponding nadir Pepi swings of -4.0±2.6 cmH₂O. With OA and CPAP combination therapy, a CPAP level of 2.3±0.9 cmH₂O abolished respiratory events and resulted in further reduction of the nadir Pepi swings to -2.7±1.1 cmH₂O.

CONCLUSIONS:

The oral appliance device with built in airway reduces pharyngeal pressure swings and the CPAP requirements necessary to achieve stable breathing during sleep. These options may be viable alternatives for the treatment of OSA in people with high nasal resistance.

SUPPORT:

This study was supported by Oventus Medical Ltd.



Abstract ID Number 5

Poster presentation: Saturday June 3, 2017 – 10am to 10.30am

For Oventus queries email info@oventusmedical.com

www.oventusmedical.com

OM84US_May 2017

The role of a novel oral appliance therapy device on pharyngeal pressure swings and CPAP requirements during sleep in obstructive sleep apnea: A pilot study

Jason Amatoury^{1,2}, Benjamin Tong¹, Chinh Nguyen¹, Irene Szollosi³, Danny J. Eckert^{1,2}



¹Neuroscience Research Australia (NeuRA), Sydney, Australia.

²School of Medical Sciences, University of New South Wales, Sydney, Australia.

³Oventus Medical Ltd, Brisbane, Australia.



Introduction

Oral appliance therapy is often an effective alternative to continuous positive airway pressure (CPAP) for the treatment of obstructive sleep apnea (OSA). However, oral appliance treatment efficacy varies and is often poorly tolerated in people with high nasal resistance. A new oral appliance device that incorporates an opening to the oral cavity (Oventus O₂Vent T) allows breathing through the device airway. This may reduce high inspiratory pressures required to drive air through the pharynx in people with nasal obstruction.


Aims

To determine: 1) pharyngeal pressure swings during sleep with and without the oral appliance therapy device and 2) the effect of the device on the CPAP requirements to minimize pharyngeal pressure swings and abolish residual respiratory events.

Methods

Participants and Study Design

- 4 individuals with suspected sleep-disordered breathing [3 male, 1 female; age: 43-62 yrs, BMI: 28-33 kg/m²]

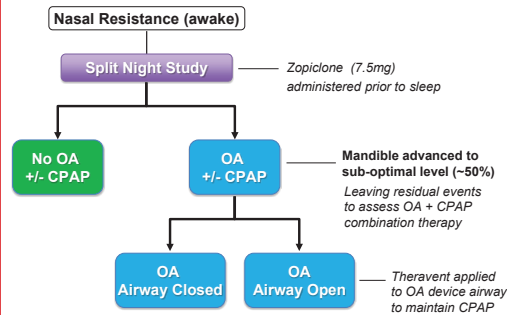

OA = oral appliance

Experimental Setup and Measurements

- Subjects were fitted with a nasal CPAP mask with a pneumotachograph (Hans-Rudolph 3700A) in series to measure flow. Mask pressure (Pmask) was also measured (Validyne DP-45)
- Choanal pressure (Pcho) & pharyngeal pressure (Pph; level of the epiglottis) were measured using pressure transducer-tipped catheters (Millar MPC-500)

Data Analysis

Nasal Resistance (Rnasal)

- Measured awake during quiet breathing supine
- Quantified at Flow = 0.2 l/s by:

$$R_{nasal} = \frac{P_{mask} - P_{cho}}{Flow}$$

Pharyngeal Pressure Swings

- Negative pharyngeal pressure swings (see Figure 2A) were averaged over 10-15 mins of stable NREM sleep for each condition

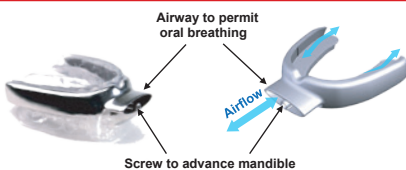


Figure 1: Oral Appliance Device

Image (left) and schematic (right) of the novel oral appliance device (Oventus O₂Vent T) used in this study. The device advances the mandible and provides the option for oral breathing via the device airway.

Results

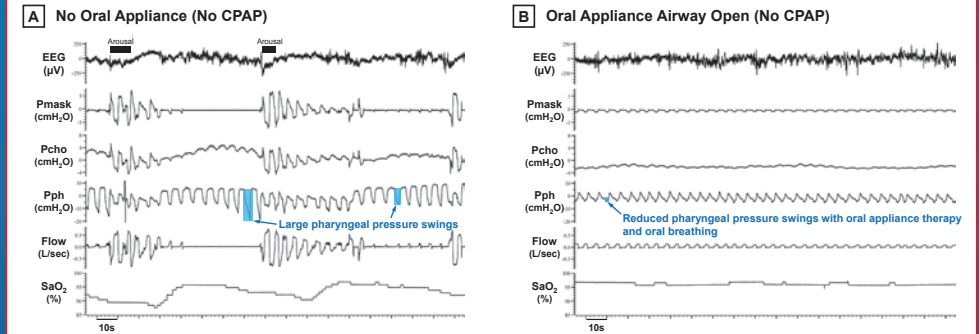


Figure 2: Raw Data with and without Oral Appliance Device

Raw data recordings from a single subject during NREM sleep under conditions of A) no oral appliance and no CPAP and B) oral appliance airway open and no CPAP. Note the large decrease in pharyngeal pressure (Pph) swings and normalization of respiratory events with the oral appliance airway open (B) compared with no oral appliance (A). Pmask = mask pressure. Pcho = choanal pressure. SaO₂ = oxygen saturation.

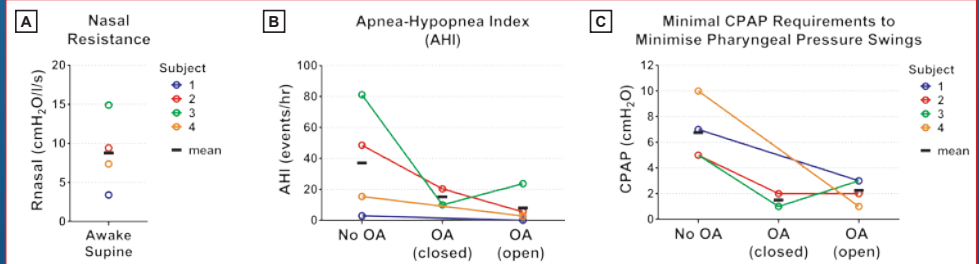


Figure 3: Nasal Resistance, AHI and Minimum CPAP Requirements

Individual subject (different color circles and lines) and mean (black bar) data for A) awake nasal resistance and B) OSA severity (apnoea-hypopnoea index [AHI]) and C) minimum CPAP requirements to minimise pharyngeal pressure swings during NREM sleep under each oral appliance (OA) condition. Note that 3/4 subjects had elevated nasal resistance (>3 cmH₂O/l/s) (A). AHI decreased with OA therapy airway closed (n=2) and was even lower with OA airway open (except subject 3). Similarly, CPAP requirements were reduced by ~66% when combined with OA therapy airway open.

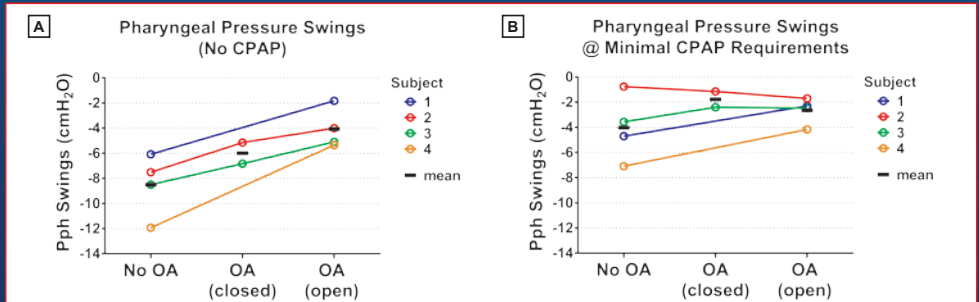


Figure 4: Pharyngeal Pressure Swings

Pharyngeal pressure swings for each oral appliance (OA) condition with A) No CPAP and B) CPAP at minimum required levels (from Figure 3C). Pharyngeal pressure swings were reduced with OA therapy, and were lowest during OA airway open, i.e. ~52% decrease OA (open) vs. No OA (A). The reduction in pharyngeal pressure swings during OA airway open was similar to CPAP alone (B, No OA condition). When combined with CPAP, OA therapy decreased pharyngeal pressure swings further, i.e. ~68% decrease for OA (open)+CPAP (B) vs. No OA (No CPAP) (A).

Summary and Conclusion

During sleep, the oral appliance with built-in airway:

- ↓ Pharyngeal pressure swings
 - ↓ CPAP level required to abolish respiratory events & achieve stable breathing
- The oral appliance device alone or combined with CPAP may be viable alternatives for the treatment of OSA in people with high nasal resistance.

Acknowledgements

This study was supported by Oventus Medical Ltd.

